

### Bio-Lever <BL-RC150VB-C1> for Force curve measurement of Bio samples


#### Characteristics

- Two types of cantilevers suitable for force curve measurements of bio samples.  
 A lever (60um long) : Low noise cantilever  
 B lever (100um long) : Small spring constant cantilever
- Gold on both sides of cantilever  
 Gold coating on the tip side makes functionalizing the tip easier (e.g., using thiol chemistry)
- The tip is located at the very end of the cantilever.  
 Since the tip isn't hidden by the body of cantilever, it can be positioned exactly at a point of interest using an optical microscopy.
- V-shaped tip of sharp and tall.  
 The radius of curvature of the tip is 40nm or less (30nm typ.). The tip height is greater than 5um high to help preventing the body of the cantilever from touching a specimen.
- Pre-separated chips offered in Gel-Pak case (picture left)  
 24chips / unit



#### Cantilever

The rectangular silicon nitride cantilevers with both-side gold coating show the mechanical properties below. A lever is the shortest and B lever is the softest cantilever commercially available (as of Aug. 2001).

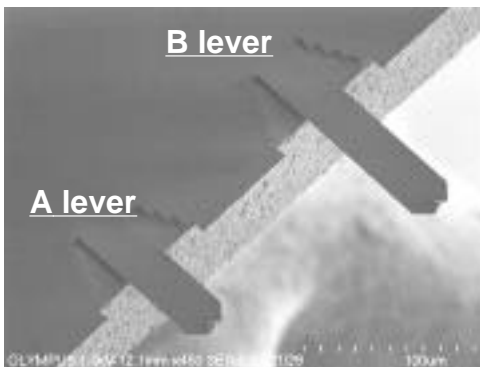

	A lever	B lever
Length x width	60um x 30um	100um x 30um
Thickness	180nm (incl. gold coating)	
Resonant Freq.	37 kHz	13 kHz
Spring const.	30 pN/nm (0.03 N/m)	6 pN/nm (0.006 N/m)

Lever and tip material


Silicon nitride

Thickness of gold coating

tip side 20 nm  
 Reflex 30 nm


#### Tip

SEM micrograph around the tip observed from the tip side

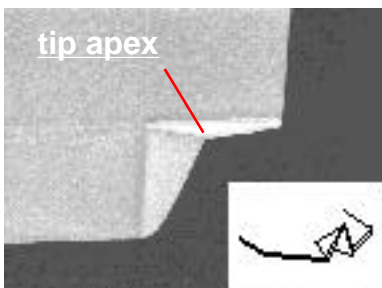


The OLYMPUS V-shaped tip is stably shaped even with the 7um-height tip (typ.). The V-shaped tip is unique. Geometrically, it is a hollow pyramid sliced in half vertically with a sharpened apex.

tip height	> 5um, 7um(typ.)
tip radius	< 40nm, 30nm(typ)
tip angle	< 45 deg. (side) < 90 deg. (front)

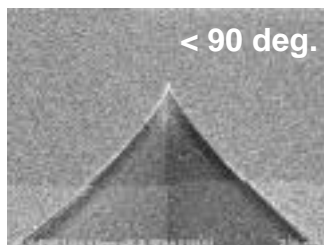


What type of the cantilever is suitable for force curve measurements ?

To generate force curve in scanning probe microscopy, the cantilever probe is to go up and down against the sample as illustrated below. You can get the information of the sample as hardness, adhesiveness and folding force of the protein molecule etc. by monitoring the cantilever deflection.

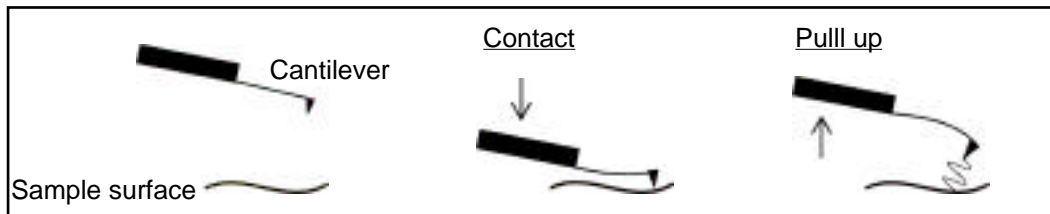

Soft cantilever (small spring constant) is requested to measure a weak force act in soft samples as bio samples. OLYMPUS achieves the small spring constant less than 10pN/nm with B lever of the Bio-Lever.

The left chart is the thermal vibration spectrum of the B lever at room temperature. The resonant frequency is 12 kHz and the spring constant is estimated at 3pN/nm by thermal method.

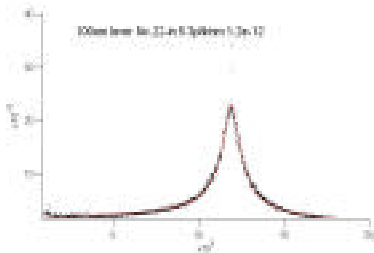


In force curve measurements, thermal noise of the cantilever itself should be small. As Brownian motion of particles in water, that is well known phenomena, the cantilever vibrates thermally. This is a mechanical noise which worsens the S/N ratio of the force measurement.

Short cantilever is the solution for lowering the noise level. When the spring constant is the same, the shorter cantilever shows less thermal noise in the band width of the SPM instrument.

The A lever of the OLYMPUS Bio-Lever (60um long) is the shortest cantilever available in the market and shows the spring constant of 30pN/nm (typ.).

As a practical application of lower noise measurements to single molecule force measurements, graph (right) shows a measurement of the B-S transition in lambda digest DNA in PBS solution. The noise level is obviously lower than the step in the middle of the curve of around 55pN.

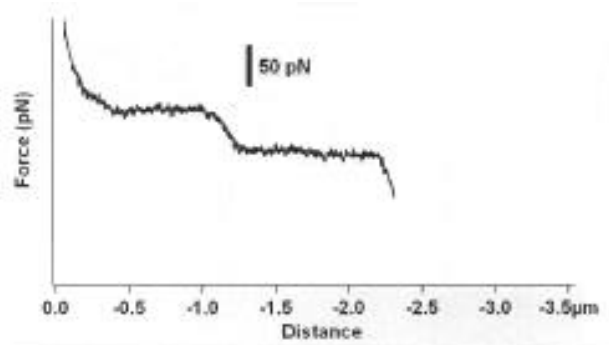

Courtesy of Dr.R.Proksch, Asylum Research



Atomic Force F&E GmbH  
 Hauptstrasse 161 DE-68259 Mannheim  
 Phone: +49-621-762117-0 / Fax: +49-621-762117-11 / e-mail: info@af-fe.de